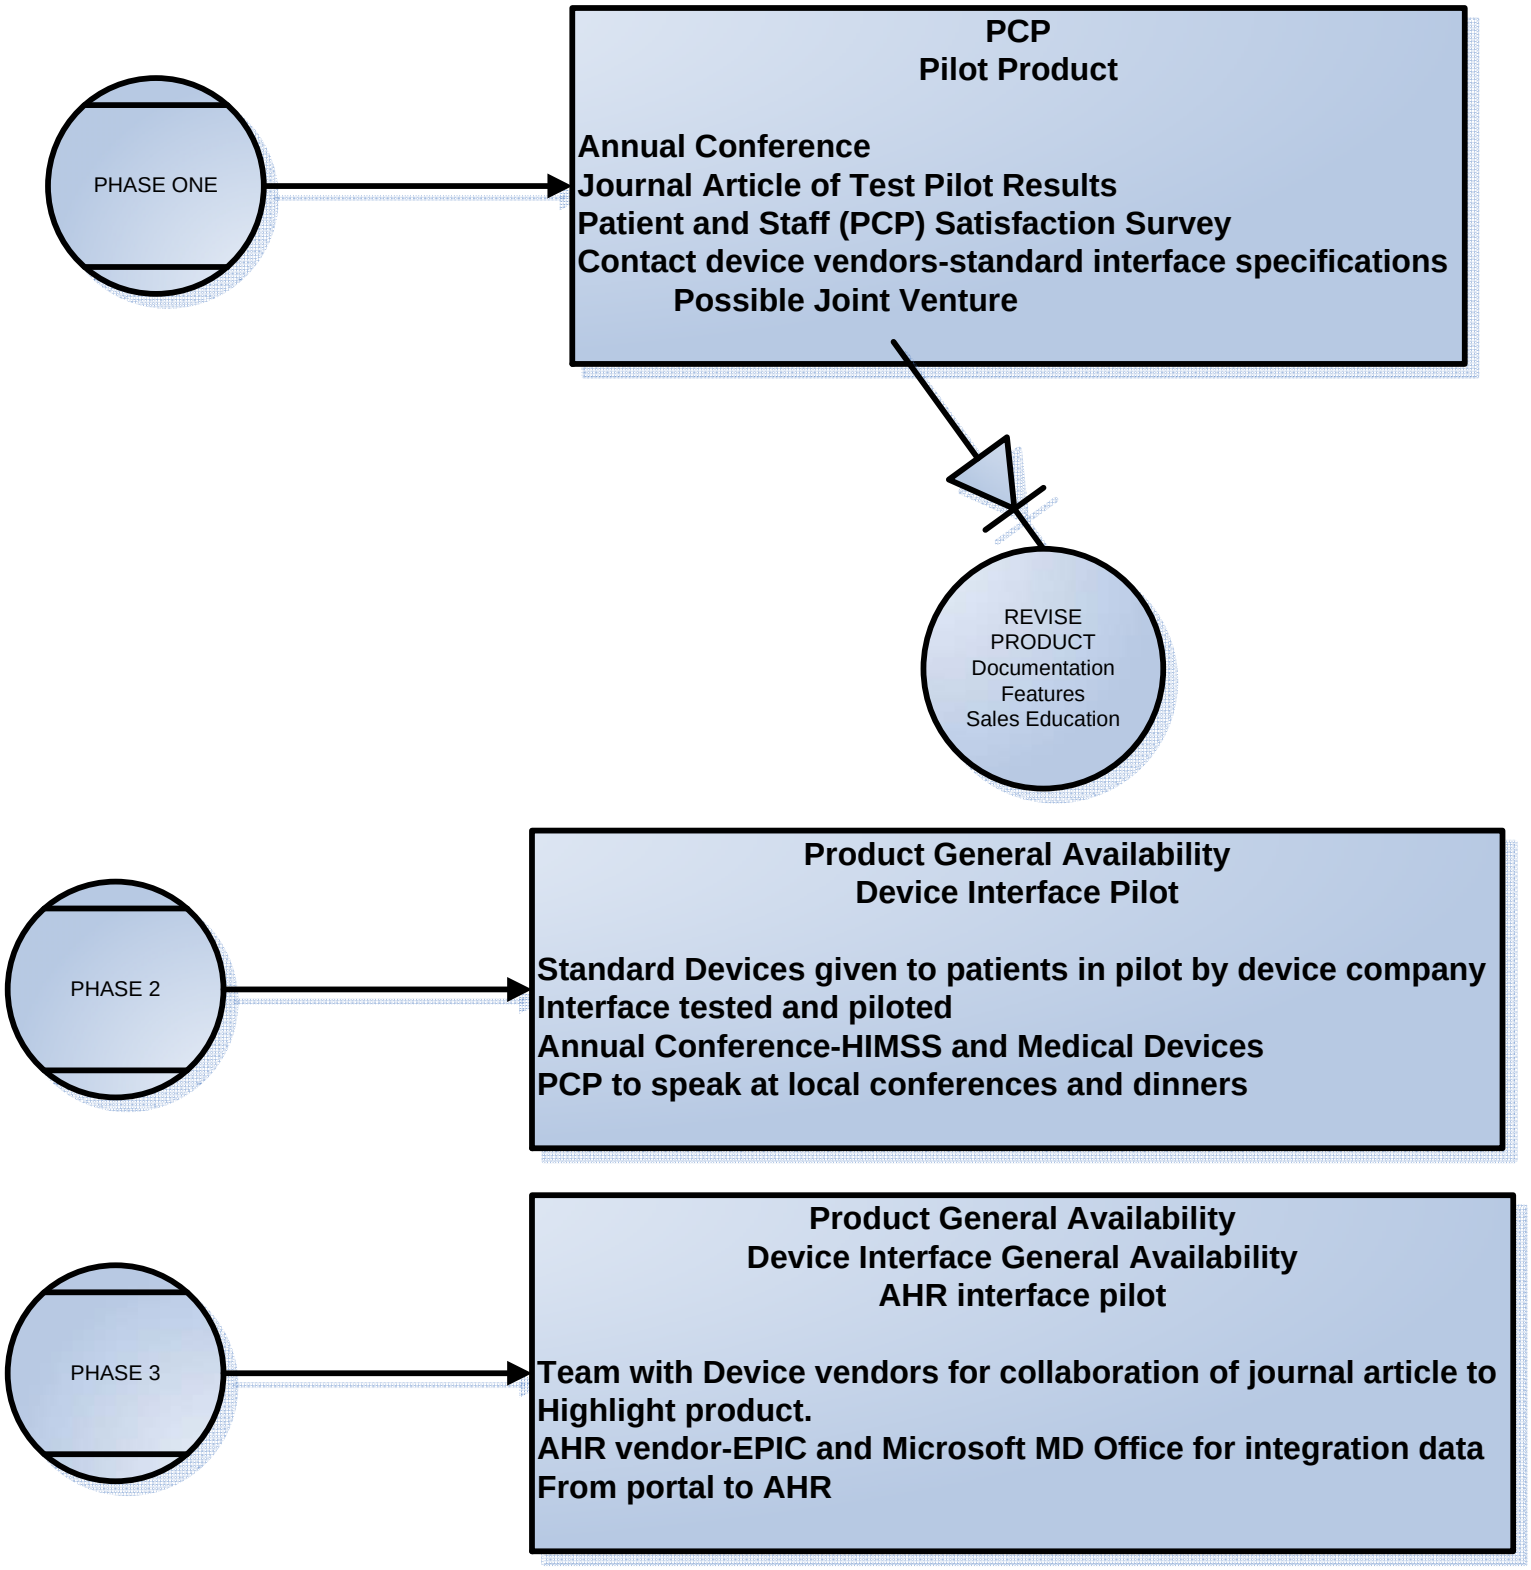
PHASE ONE
PCP
Pilot Product
Annual Conference
Journal Article of Test Pilot Results
Patient and Staff (PCP) Satisfaction Survey
Contact device vendors-standard interface specifications
Possible Joint Venture
REVISE
PRODUCT
Documentation
Features
Sales Education
PHASE 2
Product General Availability
Device Interface Pilot
Standard Devices given to patients in pilot by device company
Interface tested and piloted
Annual Conference-HIMSS and Medical Devices
PCP to speak at local conferences and dinners
PHASE 3
Product General Availability
Device Interface General Availability
AHR interface pilot
Team with Device vendors for collaboration of journal article to
Highlight product.
AHR vendor-EPIC and Microsoft MD Office for integration data
From portal to AHR